




www.peaklaboratories.com

30 PPV H₂ and C₂H₂ using the Peak Performer 1 RCP (atmospheric samples and UHP applications use same PP1 model)

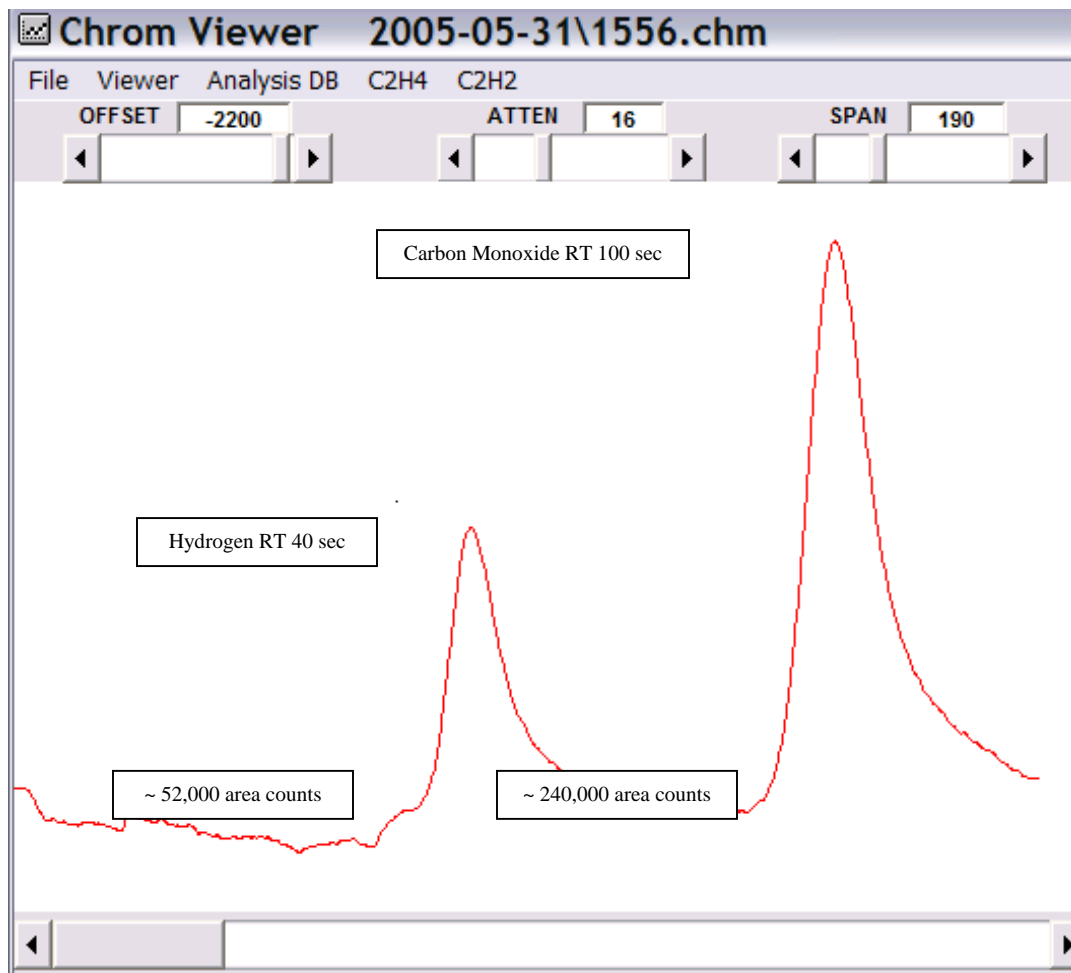

Sample - 1 ppmv N₂ standard blended to 30 ppbv using Peak Span Gas Blender
Detector - Peak Labs Reducing Compound Photometer (RCP) @ 265 C
Carrier - Purified N₂ @ 20 sccm
Column - Unibeads 1S + MS 13X