


25 PPBV BTEX using the Peak Performer 1 RCP (benzene, toluene, backflush ethylbenzene, o,m,p-xylene)

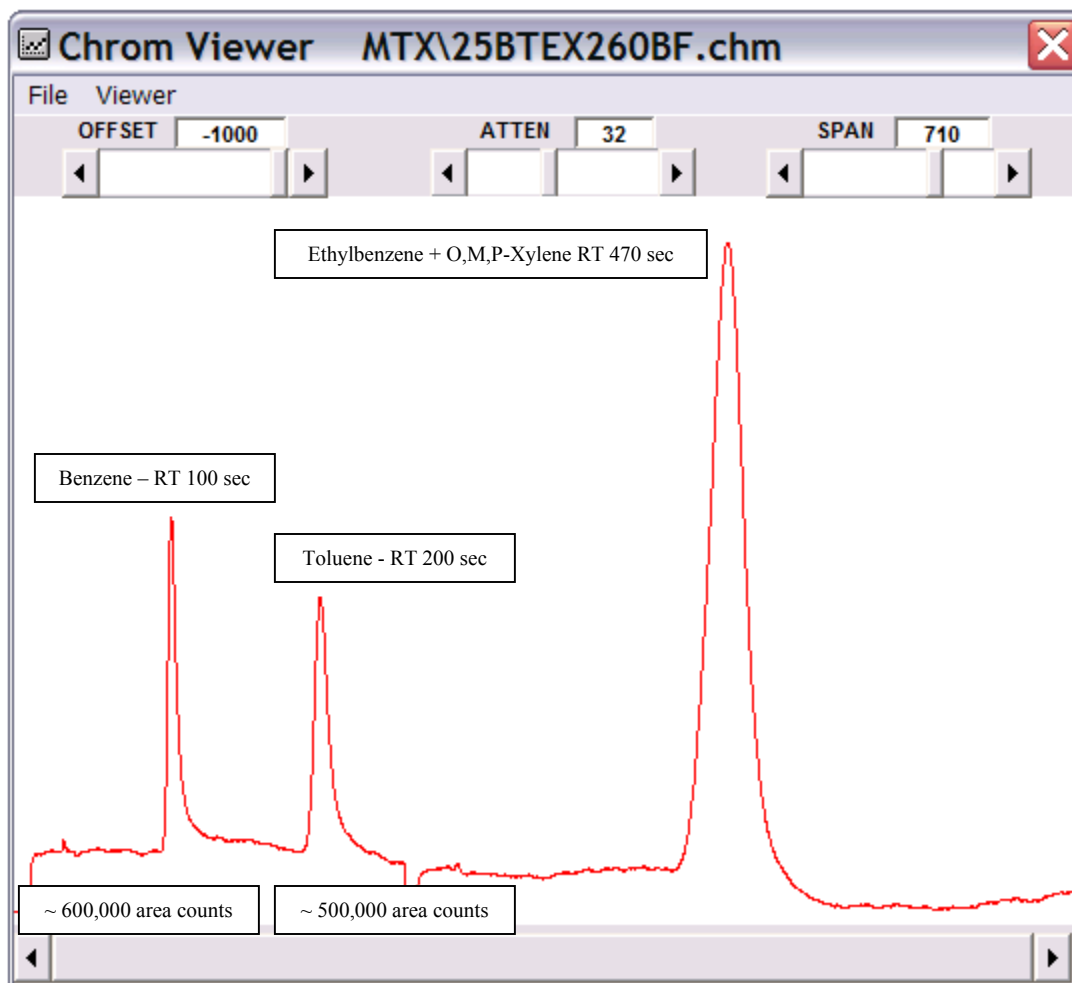

Sample - 10 ppmv N2 standard blended to 25 ppbv using Peak Span Gas Blender
Detector - Peak Labs Reducing Compound Photometer (RCP) @ 265 C
Carrier - Purified N2 @ 25 sccm
Column - Restek™ MXT-200